


INSTRUCTION MANUAL

POCKET AUTORANGING DMM

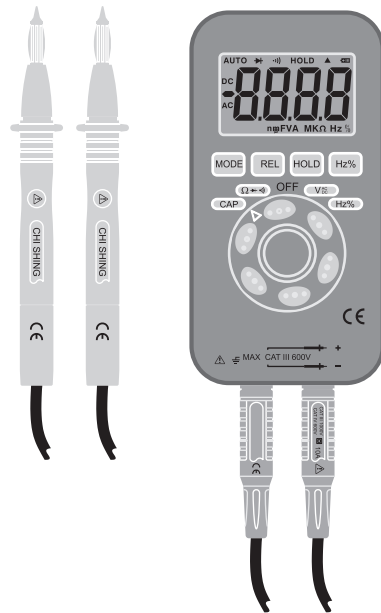

1.Safety

International Safety Symbols

- This symbol, adjacent to another symbol or terminal, indicates the user must refer to the manual for further information.
- This symbol advises the user that the terminal(s) so marked must not be connected to a circuit point at which the voltage with respect to earth ground exceeds (in this case) 600 VAC or VDC.
- Double insulation


2.Safety Precautions

- Improper use of this meter can cause damage, shock, injury or death. Read and understand this users manual before operating the meter.
- Make sure any covers or battery doors are properly closed and secured.
- Always disconnect the test leads from any voltage source before replacing the battery or fuses.
- Do not exceed the maximum rated input limits.
- Use great care when making measurements if the voltages are greater than 25VAC rms or 35VDC. These voltages are considered a shock hazard.
- Always discharge capacitors and remove power from the device under test before performing Capacitance, Diode, Resistance or Continuity tests.
- Remove the battery from the meter if the meter is to be stored for long periods.

3.Description

Meter Description


- 1.3 3/4 Digit (4000 count)
- 2.REL button
- 3.MODE button
- 4.HOLD button
- 5.Hz% button
- 6.Function switch
- 7.Battery cover
- 8.COM input jack
- 9.Positive input jack

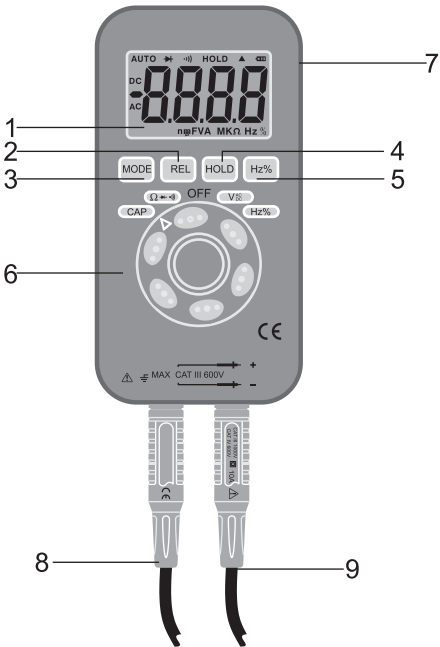

4.Specifications

Electrical Specifications

Function	Range	Accuracy
DC Voltage	400.0mV	$\pm(0.7\% \text{ rdg} + 3\text{d})$
	4.000V, 40.00V,	$\pm(1.0\% \text{ rdg} + 3\text{d})$
	400.0V-600V	$\pm(1.3\% \text{ rdg} + 3\text{d})$
AC Voltage	4.000V, 40.00V	$\pm(1.0\% \text{ rdg} + 10\text{d})$
	40-400Hz 400.0V-600V	$\pm(2.3\% \text{ rdg} + 5\text{d})$
Resistance	400.0 Ω , 4.000k Ω , 40.00k Ω , 400.0k Ω	$\pm(2.0\% \text{ rdg} + 5\text{d})$
	4.000M Ω	$\pm(5.0\% \text{ rdg} + 5\text{d})$
	40.00M Ω	$\pm(10.0\% \text{ rdg} + 5\text{d})$
Capacitance	4.000nF	$\pm(5.0\% \text{ rdg} + 30\text{d})$
	40.00nF	
	400.0nF	$\pm(3.0\% \text{ rdg} + 15\text{d})$
	4.000 μ F, 40.00 μ F, 100.0 μ F	$\pm(10.0\% \text{ rdg} + 15\text{d})$
Frequency	5.000Hz, 50.00Hz, 5000.0Hz, 5.000kHz, 50.00kHz, 500.0kHz, 10MHz	$\pm(2.0\% \text{ rdg} + 5\text{d})$
Duty Cycle	0.1-99%	

Max input voltage	600V AC/DC
Input Sensitivity	10Vrms min. <9.999KHz
(Frequency Ranges)	40Vrms min. >99.99KHz
Diode Test	Test current 1mA max., open circuit voltage
Continuity Check	Audible signal if the resistance is <50Ω
Display	4000 count 3¾ digit LCD
Over range indication	LCD displays “OL”
Polarity	Minus (-) sign for negative polarity.
Low Battery Indication	“  ” symbol indicates low battery condition.
Battery	CR2032 3V Lithium
Operating Temperature	0°C to 40°C (32°F to 104°F)
Storage Temperature	-10°C to 50°C (14°F to 122°F)
Weight	95
Size	115x60x16mm
Standard	IEC1010 CAT II I 600V Pollution degree III, CE Approved


5. Operation

AC or DC Voltage Measurement

- Set the function switch to the “**V^{AC}**” position, press MODE Button to choose DC or AC Voltage measurements. Touch the test probe tips to the circuit under test. Be sure to observe the correct polarity (red lead to positive, black lead to negative).
- Read the voltage on the display



Resistance/Continuity Measurement

WARNING: To avoid electric shock, disconnect power to the unit under test and discharge all capacitors before taking any resistance measurements. Remove the batteries and unplug the line cords. Never measure continuity on circuits or wires that have voltage on them.

- Set the function switch to the “**Ω**  **•**” position.
- Connect the test leads to the circuit to be measured.
- Read the value on the display.
- For Continuity tests, press the MODE button until the “**•**” symbol appears in the display.
- If the resistance is less than 50 ohms, an audible tone will sound.

Diode Test

WARNING: To avoid electric shock, do not test any diode that has voltage on it.

- Set the function switch to “**Ω**  **•**” position.
- Press the MODE button once to enter Diode Test. The “ ” symbol will appear in the display.
- Touch the test probe tips to the diode or semiconductor junction you wish to test. Note the meter reading.
- Reverse the test lead polarity by reversing the red and black leads. Note this reading.
- The diode or junction can be evaluated as follows:
 - A. If one reading shows a value and the other reading shows OL, the diode is good.
 - B. If both readings show OL, the device is open.
 - C. If both readings are very small, or 0, the device is shorted

Capacitance Measurement

WARNING: To avoid electric shock, disconnect power to the unit under test and discharge all capacitors before taking any capacitance measurements. Remove the batteries and unplug the line cords. Never measure continuity on circuits or wires that have voltage on them.

- Set the function switch to the “**CAP**” position.
- Connect the test leads to the capacitor to be measured.
- Read the value on the display.

Frequency/Duty Cycle Measurement

- Set the function switch to the “**Hz%**” position.
- Press the Hz% button once to display Duty Cycle %. Pressing the button again will toggle the display to frequency (Hz).
- Touch the test probe tips to the circuit under test. Be sure to observe the correct polarity (red lead to positive, black lead to negative).
- Read the value on the display.

6. Features

Relative Button

The relative measurement feature allows you to make measurements relative to a stored reference value. A reference voltage can be stored and measurements made in comparison to that value. The displayed value is the difference between the reference value and the measured value.

- Perform the measurement as described in the operating instructions.
- Press the REL button to store the reading in the display and the “**Δ**” indicator will appear on the display.
- The display will now indicate the difference between the stored value and the measured value.
- Press the REL button to exit the relative mode.

Note: The Relative function does not operate in the Frequency function.

Hold Button

The Data Hold function allows the meter to “**FREEZE**” a measurement for later reference

- Press the “**HOLD**” button to “**FREEZE**” the display, the “**HOLD**” indicator will appear.
- Press the “**HOLD**” button to return to normal operation.

Auto Power Off

- To save power, the display automatically turns off in 30 minutes.
- Press the MODE button to turn display back on.
- To cancel Auto Power Off, set the function switch to the off position. Hold down the MODE button and turn the function switch to the desired position and release the MODE button after 3 seconds.

Maintenance

WARNING: Disconnect the test leads from any source of voltage before removing the back cover or the battery/fuse door. Do not operate your meter until the rear housing is in place and fastened securely.

Replacing the Battery

- Remove the rubber holster (if in place)
- Remove Philips head screw and lift off the rear housing of the meter.
- Replace old battery with fresh CR2032 type button battery.
- Replace the rear cover and secure the screw.



Rev. 091207